



How to use the DiaSpect Tm



Sampling



1
Disinfect and dry the puncture site



2
Make the incision on the side of the finger tip



3
Wipe away first 3 drops of blood then fill the cuvette without interruption



4
Wipe off the outside of the cuvette. Check that the cuvette is completely filled

Measuring



1
Insert the filled cuvette, press down gently and hold in position



2
The hemoglobin value will be displayed instantly



3
Pull out the cuvette quickly. Record the result as soon as the checkmark is shown




4
The result is displayed until the next measurement or until pressing down the cuvette holder

Cleaning

Use conventional solvent-free surface disinfectants, or alcohol based substances such as 70% isopropyl alcohol. Do not spray the instrument!



1
Pull the backside of the cuvette holder slightly towards you and lift up

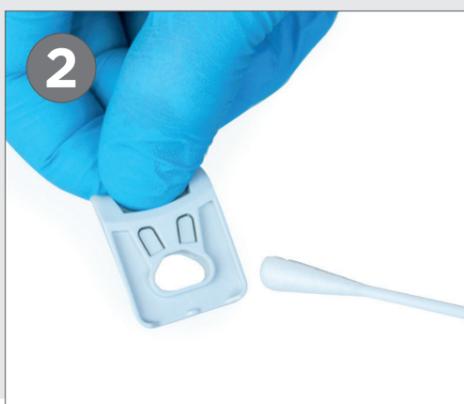

2
Clean cuvette holder with cold water or mild detergent, followed by disinfectant



3
Reinsert the dry cuvette holder by pressing down until you feel a "click"



4
Clean device with cold water or mild detergent, followed by disinfectant